


Name BBSHT
Origin Varian
Solvent dms
Number of Scans 32
Receiver Gain 54
Relaxation Delay 1.0000
Pulse Width 4.0500
Acquisition Date 2022-07-04
Spectrometer Frequency 399.89
Spectral Width 7183.9
Lowest Frequency -792.7
Nucleus 1H
Acquired Size 16384
Spectral Size 65536

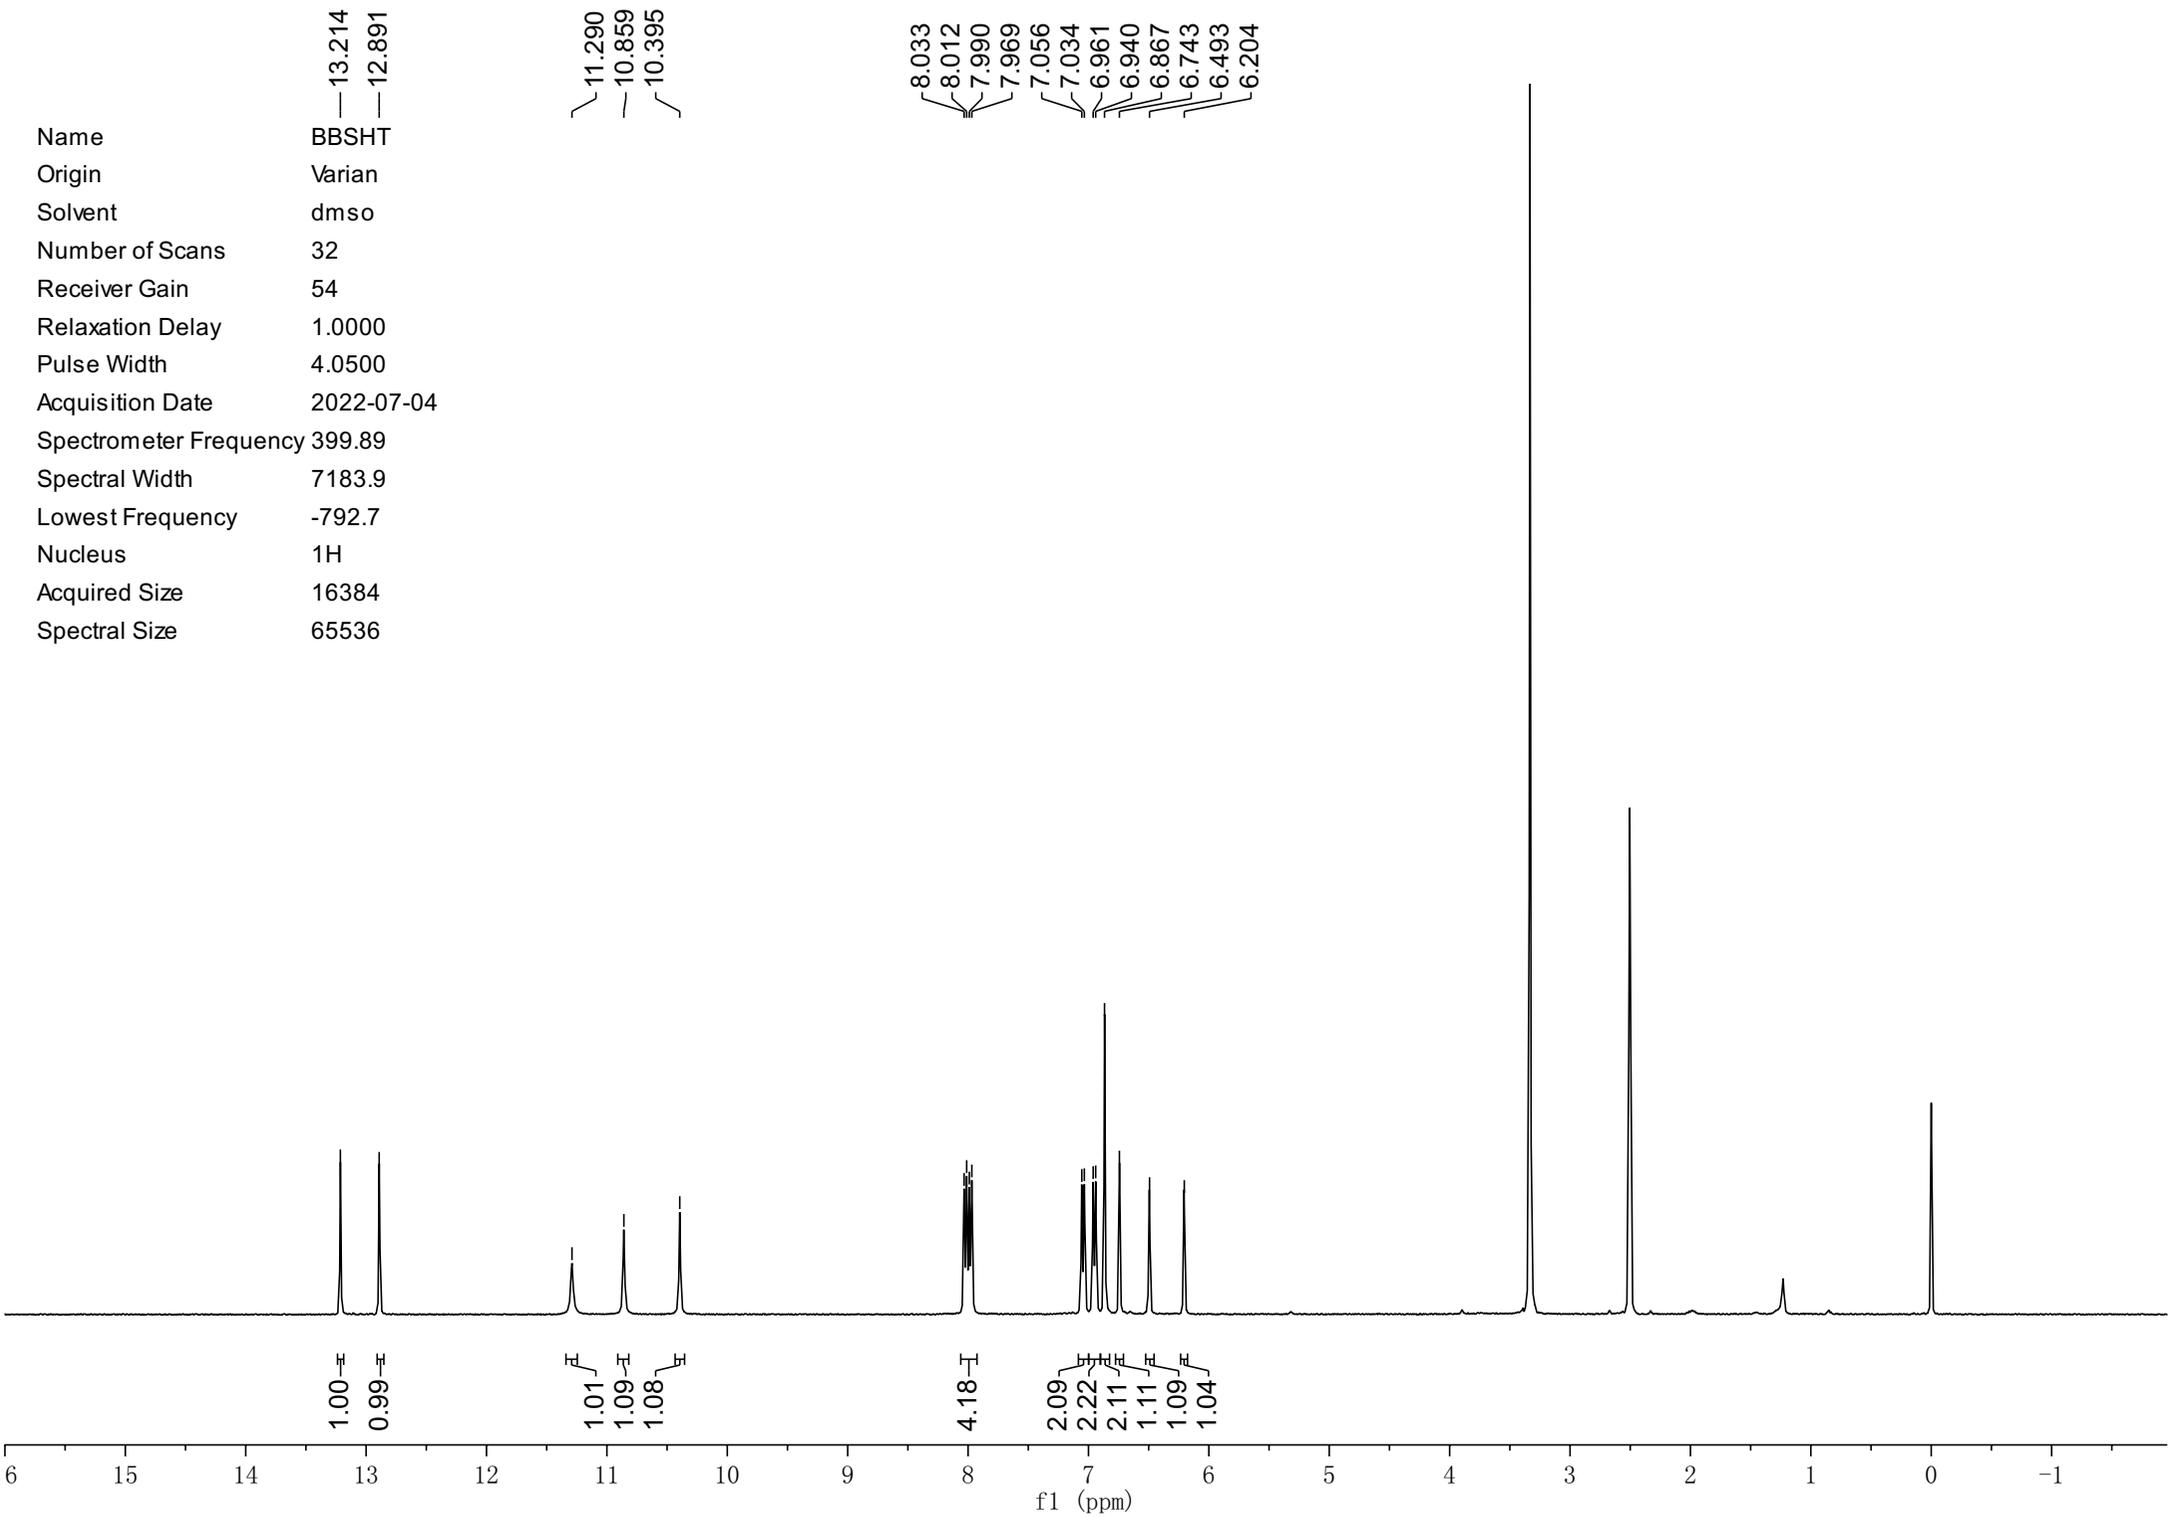

Name BBSHT
Origin Varian
Solvent dmsd
Number of Scans 32
Receiver Gain 54
Relaxation Delay 1.0000
Pulse Width 4.0500
Acquisition Date 2022-07-04
Spectrometer Frequency 399.89
Spectral Width 7183.9
Lowest Frequency -792.7
Nucleus 1H
Acquired Size 16384
Spectral Size 65536

8.033
8.012
7.990
7.969

7.056
7.034
6.961
6.940
6.867

6.743

6.493

6.204

